



Instruction manual



**EtherCAT[®] slave interface
for digital multibus
Mass Flow / Pressure instruments**

Doc. no.: 9.17.063F Date: 11-04-2012



ATTENTION

**Please read this instruction manual carefully before installing and operating the instrument.
Not following the guidelines could result in personal injury and/or damage to the equipment.**

Disclaimer

The information in this manual has been reviewed and is believed to be wholly reliable. No responsibility, however, is assumed for inaccuracies. The material in this manual is for information purposes only, and is subject to change without notice.

Bronkhorst High-Tech B.V.
December 2011

Symbols



Important information. Discarding this information could cause injuries to people or damage to the Instrument or installation.



Helpful information. This information will facilitate the use of this instrument.



Additional info available on the internet or from your local sales representative.

Warranty

Bronkhorst products are warranted against defects in material and workmanship for a period of three years from the date of shipment provided they are used in accordance with the ordering specifications and not subjected to abuse or physical damage. Products that do not operate properly during this period may be repaired or replaced at no charge. Repairs are normally warranted for one year or the balance of the original warranty, whichever is the longer.



See also paragraph 9 of the Conditions of sales:
http://www.bronkhorst.com/files/corporate_headquarters/sales_conditions/en_general_terms_of_sales.pdf

The warranty includes all initial and latent defects, random failures, and undeterminable internal causes.

It excludes failures and damage caused by the customer, such as contamination, improper electrical hook-up, physical shock etc.

Re-conditioning of products primarily returned for warranty service that is partly or wholly judged non-warranty may be charged for.

Bronkhorst High-Tech B.V. or affiliated company prepays outgoing freight charges when any party of the service is performed under warranty, unless otherwise agreed upon beforehand, however, if the product has been returned collect to our factory or service center, these costs are added to the repair invoice. Import and/or export charges, foreign shipping methods/carriers are paid for by the customer.

Table of contents

1	GENERAL PRODUCT INFORMATION	4
1.1	INTRODUCTION	4
1.2	MULTIBUS TYPES	4
1.2.1	References to other applicable documents	5
1.2.2	Manuals and user guides	5
1.2.3	Technical Drawings	5
1.2.4	Software tooling	5
1.3	SHORT FORM START-UP	6
2	FUNDAMENTALS OF ETHERCAT	7
2.1	ETHERCAT STATE MACHINE	8
3	INSTALLATION	9
3.1	INSTRUMENT OVERVIEW	9
3.2	PIN ASSIGNMENT	9
3.3	CONNECTION CABLES	10
3.4	ETHERCAT CONNECTION	10
3.5	ROUTING AND SHIELDING THE BUS CABLE	11
3.6	BUS TERMINATION	11
3.7	SECOND ADDRESS SETUP	11
4	PROTOCOLS	12
4.1	CAN APPLICATION LAYER OVER ETHERCAT (CoE)	12
4.1.1	Object Dictionary	12
4.1.1.1	Object Dictionary in device description file	12
4.1.1.2	Generated Object Dictionary	12
4.2	PROCESS DATA (PDO)	13
5	DEVICE PROFILE DS-404 SUPPORT	14
6	DIAGNOSTICS	15
6.1	ETHERCAT STATUS INDICATOR	15
6.1.1	Run indicator	15
6.1.2	Error indicator	15
7	SERVICE	16
	APPENDIX A: OBJECT DICTIONARY	17
	APPENDIX B: SI UNIT AND PREFIX SPECIFICATION	23
	APPENDIX C: NON-SI UNIT SPECIFICATION	24

1 GENERAL PRODUCT INFORMATION

1.1 INTRODUCTION

Ethernet for Control Automation Technology (EtherCAT) is an open high performance Ethernet-based field bus system. The development goal of EtherCAT was to apply Ethernet to automation applications which require short data update times (also called cycle times) with low communication jitter (for synchronization purposes) and low hardware costs. Bronkhorst¹⁾ implemented EtherCAT on its instruments.



Typical automation networks are characterized by short data length per node, typically less than the minimum payload of an Ethernet frame. Using one frame per node per cycle therefore leads to low bandwidth utilization and thus to poor overall network performance. EtherCAT therefore takes a different approach, called "processing on the fly".

With EtherCAT, the Ethernet packet or frame is no longer received, then interpreted and copied as process data at every node. The EtherCAT slave devices read the data addressed to them while the telegram passes through the device. Similarly, input data are inserted while the telegram passes through. The frames are only delayed by a fraction of a microsecond in each node, and many nodes - typically the entire network - can be addressed with just one frame.


Short cycle times can be achieved since the host microprocessors in the slave devices are not involved in the processing of the Ethernet packets to transfer the process images. All process data communication is handled in the slave controller hardware. Combined with the functional principle this makes EtherCAT a high performance distributed I/O system: Process data exchange with 1000 distributed digital I/O takes about 30 µs, which is typical for a transfer of 125 byte over 100Mb/s Ethernet. Data for and from 100 servo axis can be updated with up to 10 kHz. Typical network update rates are 1–30 kHz, but EtherCAT can be used with slower cycle times, too, if the DMA load is too high on your PC.

¹⁾ **Bronkhorst:** *This includes Bronkhorst High-Tech B.V. , Bronkhorst Cori-Tech B.V. and M+W Instruments GmbH.*

1.2 MULTIBUS TYPES

In 2000 Bronkhorst developed their first digital instruments according to the "multibus" principle. The basic pc-board on the instrument contained all of the general functions needed for measurement and control, including alarm, totalizing and diagnostic functions. It had **analog** I/O-signals and also an **RS232** connection as a standard feature. In addition to this there is the possibility of integrating an interface board with **DeviceNet™**, **Profibus-DP®**, **Modbus** or **FLOW-BUS** protocol. The first generation (**MBC-I**) was based on a 16 bit Fujitsu controller. It was superseded in 2003 by the Multibus type 2 (**MBC-II**). This version was also based on the 16 bit Fujitsu controller but it had several improvements to the MBC-I. One of them is the current steering of the valve. It reduced heat production and improved control characteristics. The latest version Multibus controller type 3 (**MBC3**) is introduced in 2011. It is build around a 72MHz 32 bit NXP ARM controller. It has AD and DA controllers on board which makes it possible to measure noise free and control valves without delays. The internal control loop runs 6 times faster compared to the MBC-II therefore control stability has improved significantly. It also has several improved functions like reverse voltage protection, inrush current limitation and overvoltage protection.


MBC3 instruments can be recognised by the "MBC3" placed on lower left side of the instrument label (see example).

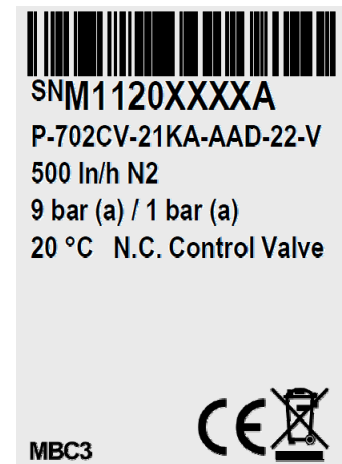

1.2.1 References to other applicable documents

Manuals and guides for digital instruments are modular. General instructions give information about the functioning and installation of instruments. Operational instructions explain the use of the digital instruments features and parameters. Field bus specific information explains the installation and use of the field bus installed on the instrument.

1.2.2 Manuals and user guides:

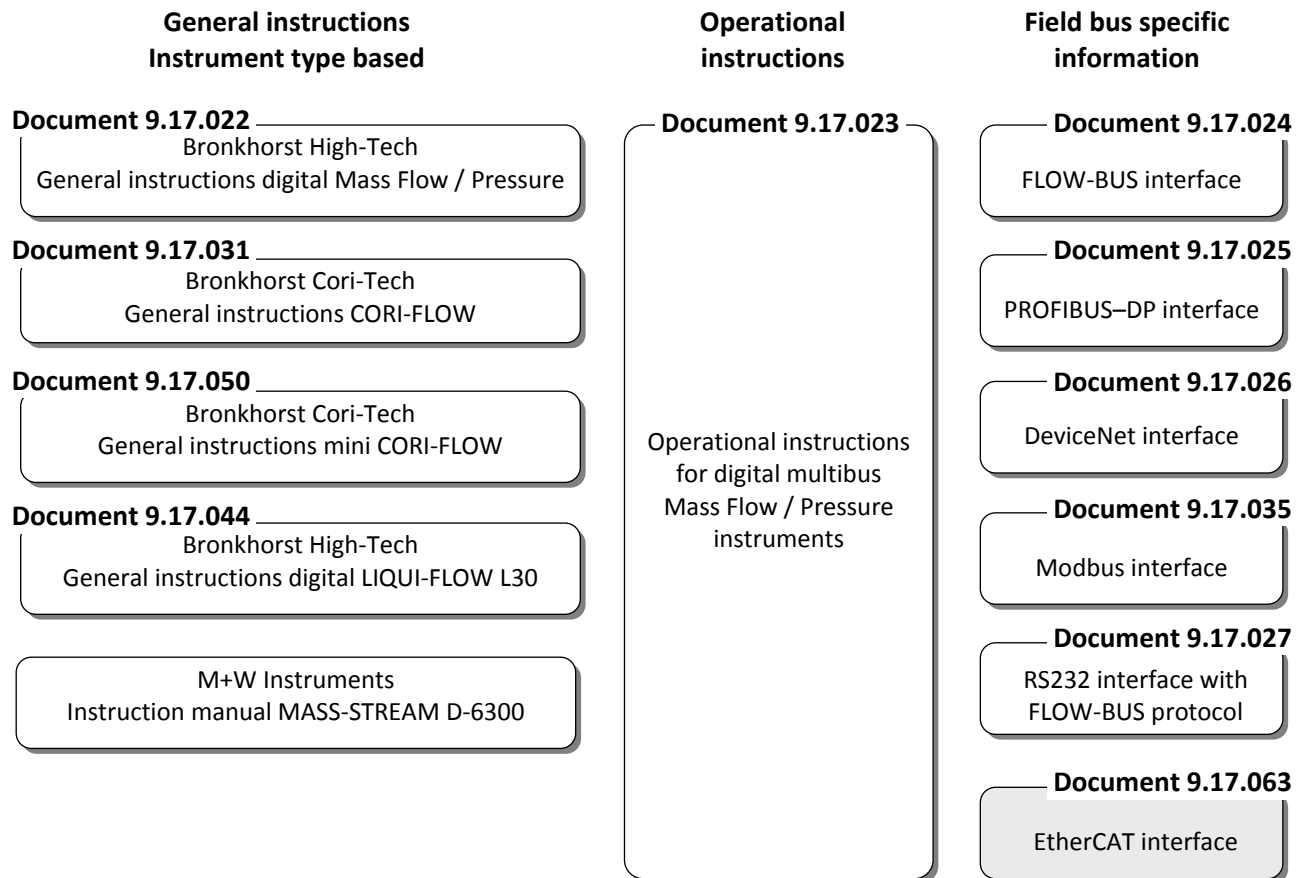

1.2.3 Technical Drawings:

Hook-up diagram laboratory-style EtherCAT (document nr. 9.16.098)

1.2.4 Software tooling:

Flowfix
FlowDDE




All these documents can be found at:
<http://www.bronkhorst.com/en/downloads>

1.3 SHORT FORM START-UP


All necessary settings for this module are already performed at Bronkhorst.

To follow next steps carefully is the quickest way to get this module operational in your own EtherCAT environment.

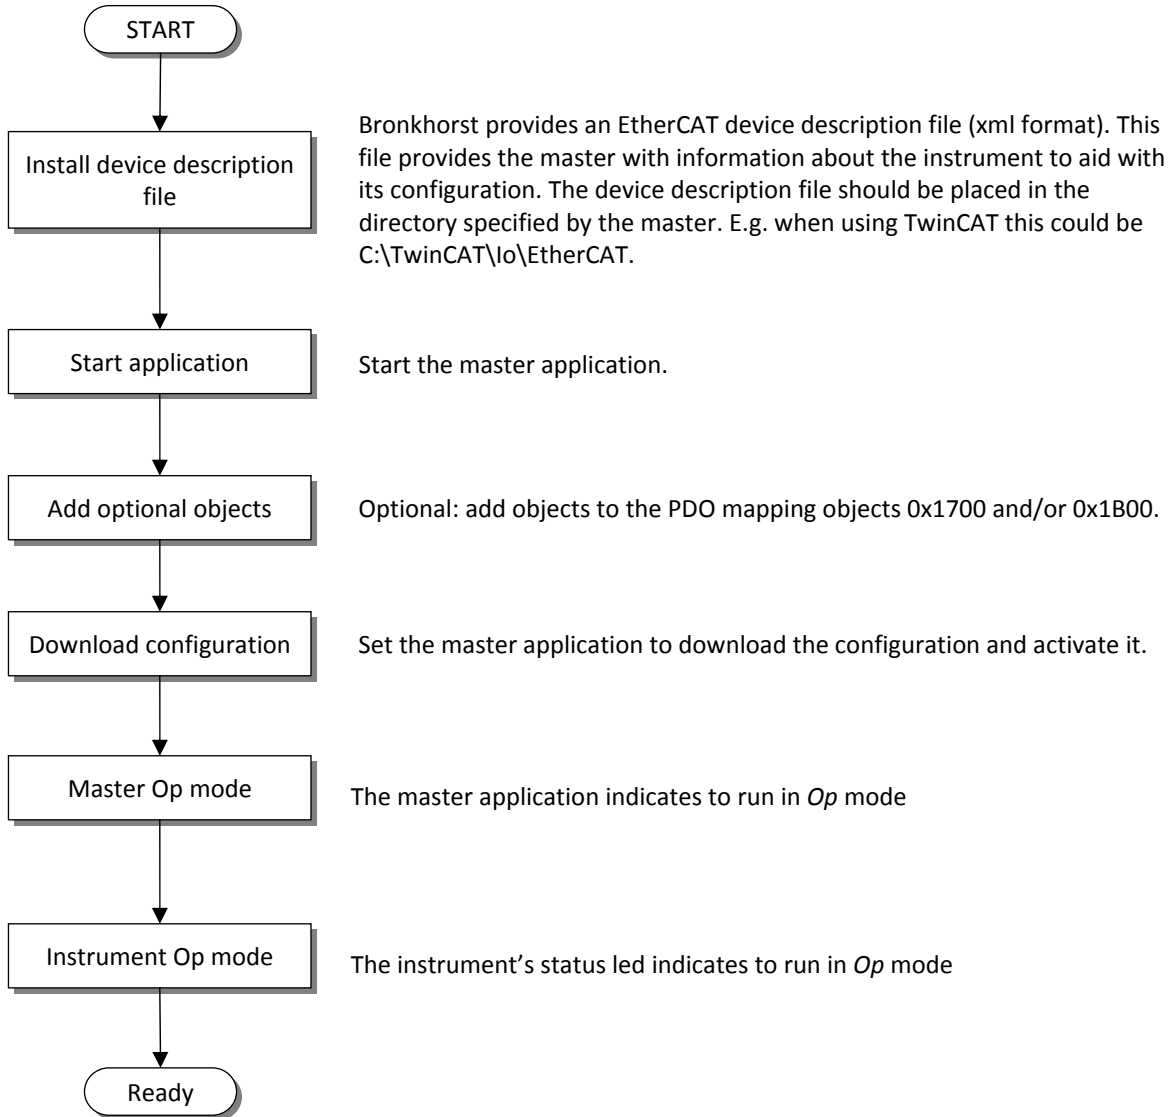


2 FUNDAMENTALS OF ETHERCAT

The EtherCAT protocol transports data directly within a standard Ethernet frame without changing its basic structure. When the master controller and slave devices are on the same subnet, the EtherCAT protocol merely replaces the Internet Protocol (IP) in the Ethernet frame.

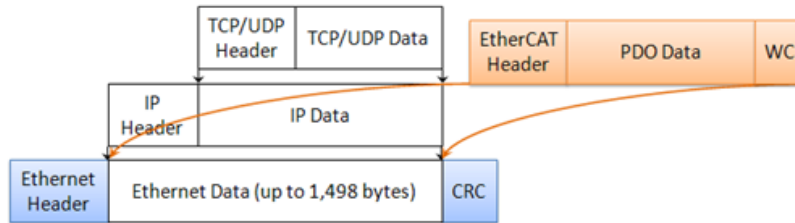


Data is communicated between master and slaves in the form of process data objects (PDOs). Each PDO has an address to one particular slave or multiple slaves, and this “data and address” combination (plus the working counter for validation) makes up an EtherCAT telegram. One Ethernet frame can contain multiple telegrams, and multiple frames may be necessary to hold all the telegrams needed for one control cycle.

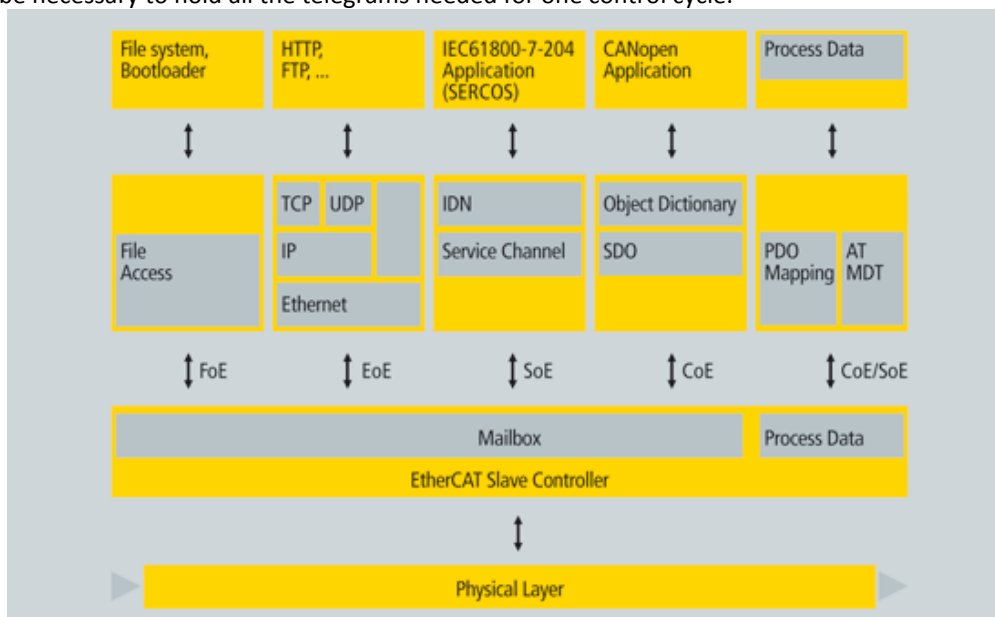

Several Device Profiles and Protocols can co-exist side by side

With some real-time protocols, the master controller sends a data packet and must wait for the process data to be interpreted and copied at every slave node. However, this method of determinism may be difficult to sustain because the master controller must add and manage a certain amount of processing time and jitter per slave. EtherCAT technology overcomes these system limitations by processing each Ethernet frame on the fly. For example, suppose the Ethernet frame is a moving train, and the EtherCAT telegrams are train cars. The bits of PDO data are people in the cars who can be extracted or inserted by the appropriate slaves. The whole “train” passes through all the slave devices without stopping, and the end slave sends it back through all the slaves again.

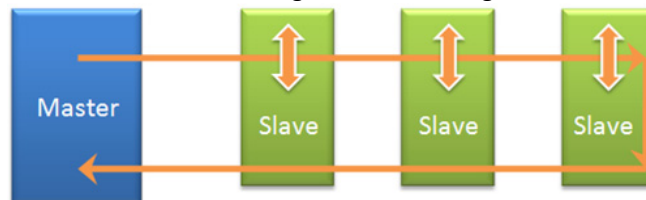

In the same way, when device 1 encounters the Ethernet packet sent by the master, it automatically begins streaming the packet to device 2, all while reading and writing to the packet with only a few nanoseconds delay. Because the packet continues passing from slave to slave to slave, it could exist in multiple devices at the same time. What does this mean practically? Let’s say you have 50 slave devices, and different data is sent to each slave. For non-EtherCAT implementations, this may mean sending out 50 different packets. For EtherCAT, one long packet that touches all slaves is sent, and the packet contains 50 devices worth of data. However, if all the slaves need to receive the same data, one short packet is sent, and the slaves all look at the same part of the packet as it is streaming through, optimizing the data transfer speed and bandwidth.


2.1 ETHERCAT STATE MACHINE

The state of the EtherCAT slave is controlled via the EtherCAT State Machine (ESM). Depending upon the state, different functions are accessible or executable in the EtherCAT slave. Specific commands must be sent by the EtherCAT master to the device in each state, particularly during the boot-up of the slave.

A distinction is made between the following states:

- Init
- Pre-Operational
- Safe-Operational
- Operational
- Bootstrap

The regular state of each EtherCAT slave after boot-up is the Operational state.

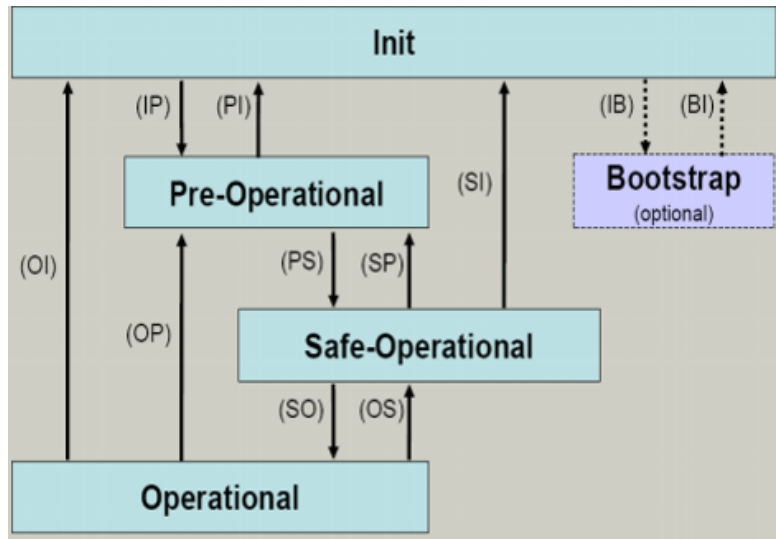

Init

After power-on the EtherCAT slave is in the *Init* state. No mailbox or process data communication is possible. The EtherCAT master initializes sync manager channels 0 and 1 for mailbox communication.

Pre-Operational (Pre-Op)

During the transition between *Init* and *Pre-Op* the EtherCAT slave checks whether the mailbox was initialized correctly. In *Pre-Op* state mailbox communication is possible, but not process data communication. The EtherCAT master initializes the sync manager channels for process data (from sync manager channel 2), the FMMU channels and PDO mapping or the sync manager PDO assignment.

Safe-Operational (Safe-Op)

During transition between *Pre-Op* and *Safe-Op* the EtherCAT slave checks whether the sync manager channels for process data communication are correct. Before it acknowledges the change of state, the EtherCAT slave copies current input data into the associated DP-RAM areas of the EtherCAT slave controller (ECSC). In *Safe-Op* state mailbox and process data communication is possible, although the slave keeps its outputs in a safe state, while the input data are updated cyclically.

Operational (Op)

Before the EtherCAT master switches the EtherCAT slave from *Safe-Op* to *Op* it must transfer valid output data. In the *Op* state the slave copies the output data of the masters to its outputs. Process data and mailbox communication is possible.

Bootstrap


In the *Bootstrap* state the slave firmware can be updated. The *Bootstrap* state can only be reached via the *Init* state. In the *Bootstrap* state mailbox communication via the *file access over EtherCAT* (FoE) protocol is possible, but no other mailbox communication and no process data communication





Bronkhorst EtherCAT instruments do not support the Bootstrap state.

3 INSTALLATION

3.1 INSTRUMENT OVERVIEW

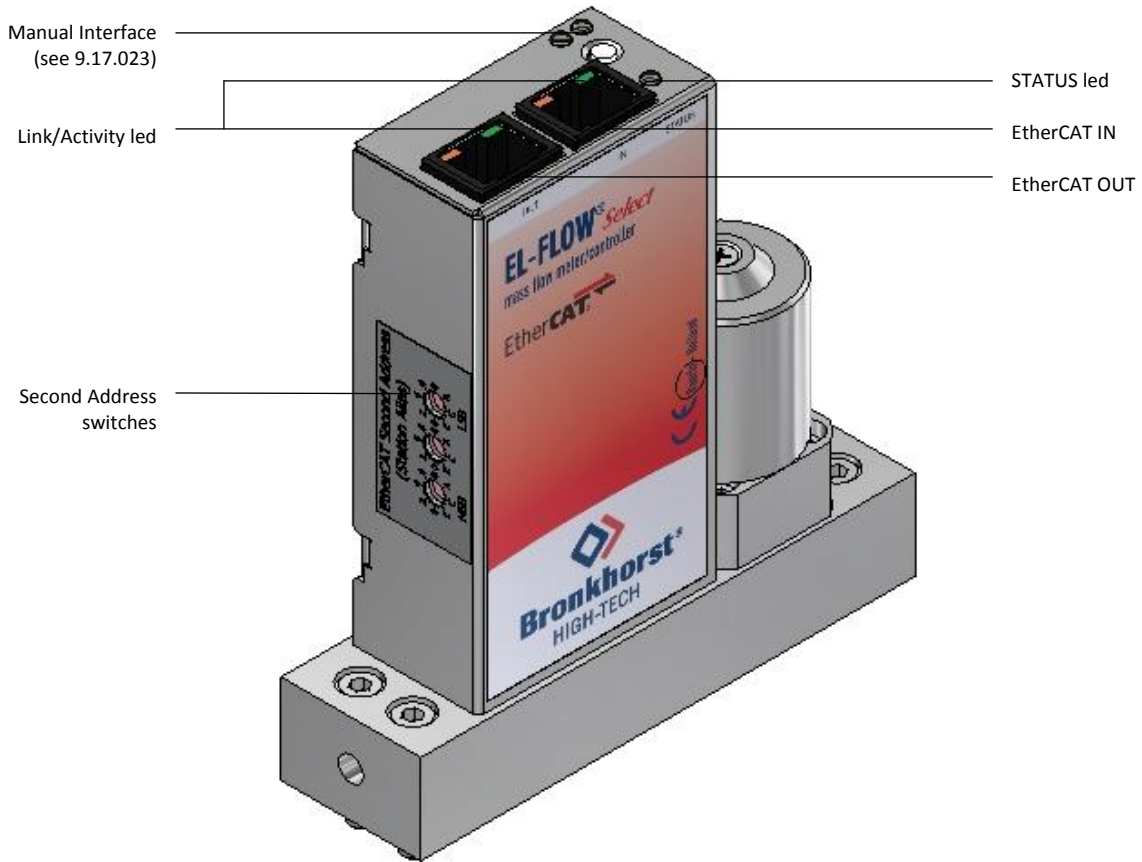


3.2 PIN ASSIGNMENT

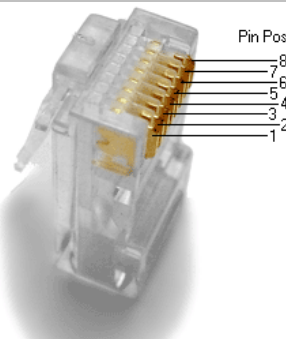RJ45 Connector	Receptacle	Pin number	Description
		1	Transmit +
		2	Transmit -
		3	Receive +
		4	Not used
		5	Not used
		6	Receive -
		7	Not used
		8	Not used

3.3 CONNECTION CABLES

Ethernet patch or crossover FTP or SFTP cables in CAT5e quality can be used as the connection cables. Lengths of 0.15 to 100 m are permitted for an EtherCAT network.

If you want to make the cables yourself, be sure to select a suitable crimp tool. Afterwards check the quality with a cable tester to avoid transmission problems.

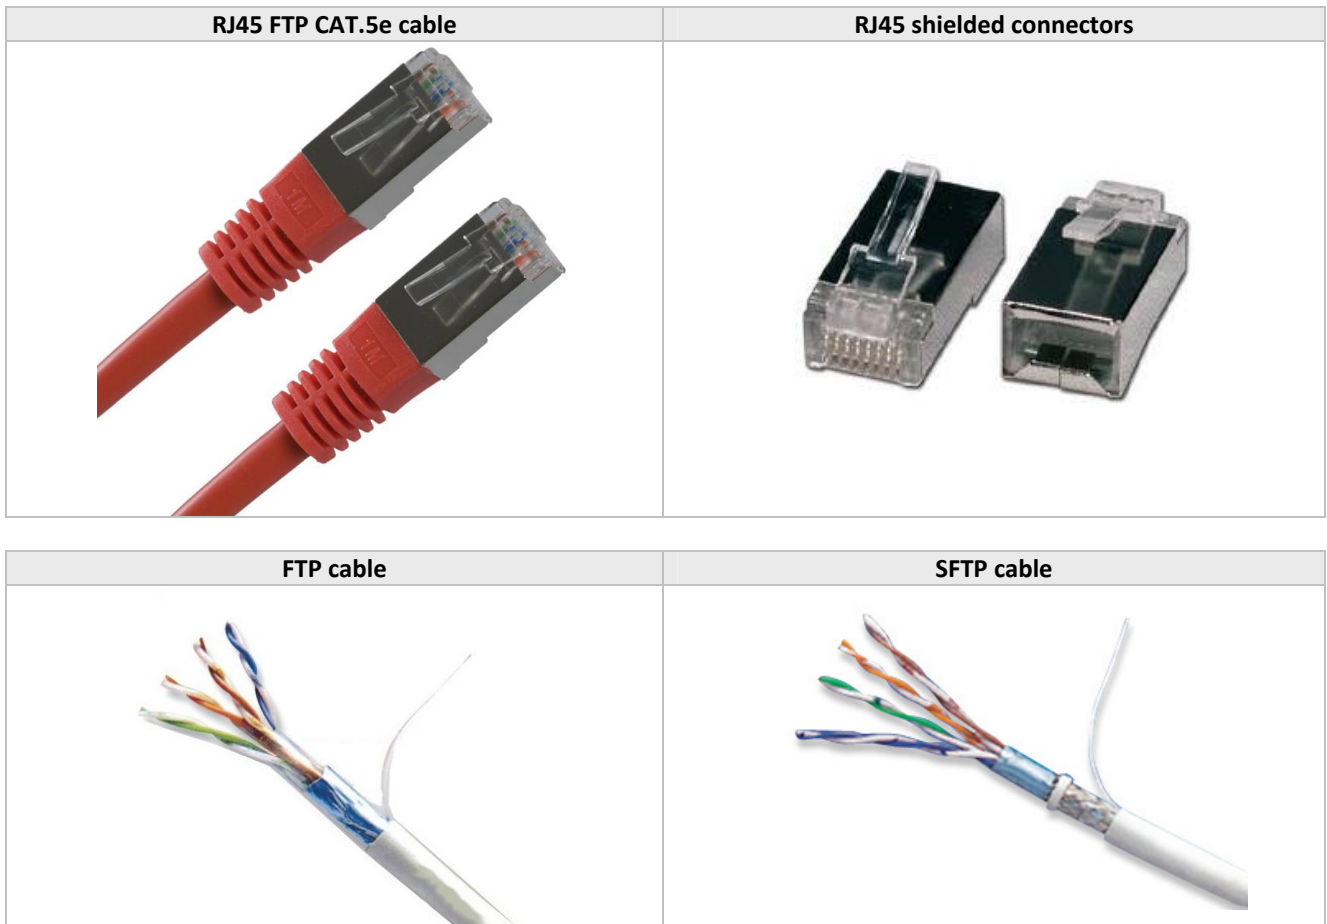

*CAT.5e cables are available with a wire of:
26AWG (wire diameter 0.140mm², with a resistance of 137 Ohm/km).
24AWG (wire diameter 0.205mm², with a resistance of 86 Ohm/km).*



*More information about cat.5e cables can be found at:
http://en.wikipedia.org/wiki/Category_5_cable*

3.4 ETHERCAT CONNECTION

The Bronkhorst instruments are equipped with a linear bus structure with two RJ45 connectors. The EtherCAT master is connected (via EtherCAT slaves, if necessary) with a shielded, twisted pair, cable to “EtherCAT IN” (RJ45). Other EtherCAT instruments are connected via “EtherCAT OUT” (RJ45).



According to IEC 802.3 the maximum cable length for 100 MBaud Ethernet is 100m (100BaseT), e.g. between two instruments.

3.5 ROUTING AND SHIELDING THE BUS CABLE

Only use shielded cables and connection elements that also meet the requirements of category 5, class 2 according to IEC11801, edition 2.0.

Correct shielding of the bus cable attenuates electrical interference that may occur in industrial environments. The following measures ensure the best possible shielding:

- Manual tighten the mounting screws on the connectors, modules, and equipotential bonding conductors.
- Use only connectors with a metal housing or a metalized housing.
- Connect the shielding in the connector over a wide surface area.
- Apply the shielding of the bus cables on both ends.
- Route signal and bus cables in separate cable ducts. Do not route them parallel to power cables (motor leads)
- Route the signal cable and the corresponding equipotential bonding, if necessary, close to each other using the shortest possible route.
- Route the bus cable closely along existing grounding surfaces.



In case of fluctuations in the ground potential, a compensating current may flow via the bilaterally connected shield that is also connected to the protective earth (PE). Make sure you supply adequate equipotential bonding in such a case.

3.6 BUS TERMINATION

A bus terminator (e.g. using bus terminating resistors) is not necessary. If no follow-up unit is connected to an EtherCAT unit, this is automatically detected.


3.7 SECOND ADDRESS SETUP

EtherCAT supports the use of a Second Address. Bronkhorst instruments have 3 rotary switches, with which a Second Address can be set in the range of 0 – 4095 (0xFFF).

This value of the rotary switches will be copied to the Configured Station Alias register (address 0x0012:0x0013) at instrument start-up.

4 PROTOCOLS

Bronkhorst instruments support the following parts of EtherCAT: CAN application layer over EtherCAT (CoE) and Process Data (PDO).

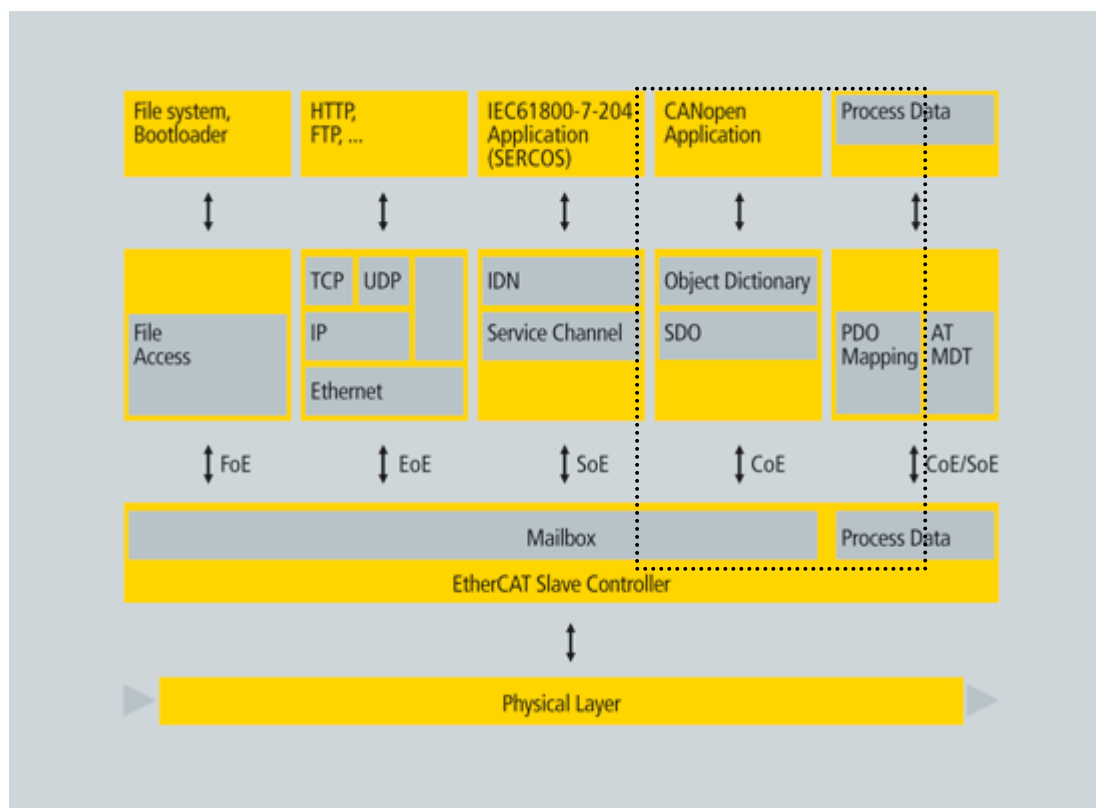

4.1 CAN APPLICATION LAYER OVER ETHERCAT (CoE)

Bronkhorst High-Tech B.V. instruments support the CAN application layer over EtherCAT (CoE) protocol. This protocol enables the exchange of data between master and slave application over EtherCAT using CANopen[®] objects. These objects are described in the Object Dictionary. The SDO protocol is used to access (read or write) the objects in the Object Dictionary.

4.1.1 Object Dictionary

The Object Dictionary consists of 2 parts:

- objects described in the device description file.
- objects generated by the instrument itself for the parameters as described in document 9.17.023.

4.1.1.1 Object Dictionary in device description file (ESI)

The objects described in the device description file are mandatory objects. These objects are listed in Appendix A: Object Dictionary. For some objects additional information about the use in Bronkhorst High-Tech B.V. instruments can be found here as well.



The current EtherCAT ESI file can be downloaded from:
http://www.bronkhorst.com/en/products/accessories/software_tools/

4.1.1.2 Generated Object Dictionary

All available parameters in Bronkhorst instruments are described in 9.17.023. These parameters are accessed by means of a process / process parameter number combination. For a selection of these parameters objects are generated and added to the Object Dictionary at instrument startup (in the range 0x2000 – 0x3000). The mapping from process / process parameter number combination to objects is done in the following way:

object index = $0x2000 + \text{process number}$
subindex = $\text{process parameter number} + 1$

Example:

DDE parameter 8: Measure has process / process parameter number combination 1 / 0. So this parameter is mapped to object index 0x2001 (= 0x2000 + 1) and subindex 1 (= 0 + 1).

For the following DDE parameters (among others) objects are generated:

8 Measure
9 Setpoint
10 Setpoint slope
21 Capacity
24 Fluid number
92 Serial number
205 fMeasure
206 fSetpoint

4.2 PROCESS DATA (PDO)

The Process Data are organized in process data objects (PDO), which are transferred using the efficient means of EtherCAT.

Objects from the Object Dictionary, which can be mapped to the PDO, can be added to the PDO Map before activating the configuration. It is possible to add 20 objects to the RxPDO Map (0x1700) and 20 objects to the TxPDO Map (0x1B00).

Which objects from the the Object Dictionary can be mapped to the PDO, can be found in Appendix A: Object Dictionary.

All objects in the range 0x2000 – 0x3000 can be mapped to the PDO, except the ones containing strings.

5 DEVICE PROFILE DS-404 SUPPORT

Bronkhorst instruments support the mandatory objects from the controller function block from CiA (draft) DS 404 V1.2, *Measurement Devices and Closed Loop Controllers*. These objects (0x6400 – 0x7405) are also listed in Appendix A: Object Dictionary

Object 0x6406 contains a representation of the unit for current value and setpoint. This representation is based on ETG.1004 *EtherCAT Unit specification*, which only contains SI units (see Appendix B: SI Unit AND Prefix Specification). Bronkhorst instruments support a lot of non-SI units, which are described in Appendix C: Non-SI Unit Specification.

The unit is represented by an unsigned32 value with the following meaning:

Prefix		Numerator		Denominator		reserved	
31	24	23	16	15	8	7	0

Examples:

kg/s is represented by

Prefix	Numerator	Denominator	reserved
0x00	0x02	0x03	0x00

with

Prefix = 0x00	means no prefix
Numerator = 0x02	means kg
Denominator = 0x03	means s

mln/min is represented by

Prefix	Numerator	Denominator	reserved
0xFD	0xC0	0x47	0x00

with

Prefix = 0xFD	means 10^{-3} = milli
Numerator = 0xC0	means ln
Denominator = 0x47	means min

6 DIAGNOSTICS

6.1 ETHERCAT STATUS INDICATOR

Bronkhorst instruments contain an EtherCAT two color status led: green and red. The led indicates the actual EtherCAT run state (green) and the actual error state (red).

The status led has several indicator states, which are applicable for both green and red. They are described in the table below.

Indicator state	Definition
on	The indicator is constantly on
off	The indicator is constantly off
blinking	The indicator is repeatedly on for 200 ms and off for 200 ms
single flash	The indicator is repeatedly on for 200 ms and off for 1000 ms
double flash	The indicator shows repeatedly a sequence of two short flashes (200 ms), separated by an off phase (200 ms), followed by a long off phase (1000 ms)

6.1.1 Run indicator

EtherCAT state	Indicator state (green)
Init	off
Pre-Operational	blinking
Safe-Operational	single flash
Operational	on

6.1.2 Error indicator

Error state	Indicator state (red)
No error	off
<ul style="list-style-type: none"> invalid state change commanded by master (e.g. from Init to Operational) request for state change to an unsupported state (e.g. Bootstrap) request for state change to an unknown state 	blinking
<ul style="list-style-type: none"> invalid mailbox configuration invalid SyncManager configuration 	single flash
Application watchdog timeout (e.g. when EtherCAT communication cable is removed)	double flash

7 SERVICE

For current information on Bronkhorst and service addresses please visit our website:

 <http://www.bronkhorst.com>


Do you have any questions about our products? Our Sales Department will gladly assist you selecting the right product for your application. Contact sales by e-mail:

 sales@bronkhorst.com

For after-sales questions, our Customer Service Department is available with help and guidance. To contact CSD by e-mail:

 support@bronkhorst.com

No matter the time zone, our experts within the Support Group are available to answer your request immediately or ensure appropriate further action. Our experts can be reached at:

 **+31 573 45 88 39**

APPENDIX A: OBJECT DICTIONARY

Index	Sub Index	Description	Data Type	Access	PDO mapping
0x1000		Device Type ¹	Unsigned32	RO	No
0x1008		Manufacturer Device Name	Visible String	RO	No
0x1009		Manufacturer Hardware Version	Visible String	RO	No
0x100A		Manufacturer Software Version	Visible String	RO	No
0x1018	0	Identity	Unsigned8	RO	No
	1	Vendor ID ²	Unsigned32	RO	No
	2	Product Code	Unsigned32	RO	No
	3	Revision Number	Unsigned32	RO	No
	4	Serial Number	Unsigned32	RO	No
0x1601	0	CO RxPDO Map	Unsigned8	RO	No
	1	Mapped Object 1	Unsigned32	RO	No
	2	Mapped Object 2	Unsigned32	RO	No
	3	Mapped Object 3	Unsigned32	RO	No
0x1700	0	RxPDO Map	Unsigned8	RW	No
	1	Mapped Object 1	Unsigned32	RW	No
	2	Mapped Object 2	Unsigned32	RW	No
	:				
	20	Mapped Object 20	Unsigned32	RW	No
0x1A01	0	CO TxPDO Map	Unsigned8	RO	No
	1	Mapped Object 1	Unsigned32	RO	No
	2	Mapped Object 2	Unsigned32	RO	No
	3	Mapped Object 3	Unsigned32	RO	No
0x1B00	0	TxPDO Map	Unsigned8	RW	No
	1	Mapped Object 1	Unsigned32	RW	No
	2	Mapped Object 2	Unsigned32	RW	No
	:				
	20	Mapped Object 20	Unsigned32	RW	No
0x1C00	0	SyncManager Communication Type	Unsigned8	RO	No
	1	Communication Type SM0	Unsigned8	RO	No
	2	Communication Type SM1	Unsigned8	RO	No
	3	Communication Type SM2	Unsigned8	RO	No
	4	Communication Type SM3	Unsigned8	RO	No
0x1C12	0	SyncManager 2 PDO Assignment	Unsigned8	RW	No
	1	PDO Mapping Table 0	Unsigned16	RW	No
	2	PDO Mapping Table 1	Unsigned16	RW	No
0x1C13	0	SyncManager 3 PDO Assignment	Unsigned8	RW	No
	1	PDO Mapping Table 0	Unsigned16	RW	No
	2	PDO Mapping Table 1	Unsigned16	RW	No
0x6400	0	CO Effective current value Xeff	Unsigned8	RO	No
	1	CO Effective current value Xeff	Float	RW	Possible

¹ Device Type = 0x00100194; this means that the controller function block of device profile DS-404 is implemented.

² Bronkhorst High-Tech B.V. Vendor ID is 1387 (0x0000056B)

Index	Sub Index	Description	Data Type	Access	PDO mapping
0x6401	0	CO Effective setpoint Weff	Unsigned8	RO	No
	1	CO Effective setpoint Weff	Float	RO	Possible
0x6402	0	CO Setpoint W	Unsigned8	RO	No
	1	CO Setpoint W	Float	RW	Possible
0x6403	0	CO 2 nd Setpoint W2	Unsigned8	RO	No
	1	CO 2 nd Setpoint W2	Float	RW	Possible
0x6404	0	CO Lower setpoint limit W0	Unsigned8	RO	No
	1	CO Lower setpoint limit W0	Float	RO	No
0x6405	0	CO Upper setpoint limit W100	Unsigned8	RO	No
	1	CO Upper setpoint limit W100	Float	RO	No
0x6406	0	CO Physical unit current value / setpoint	Unsigned8	RO	No
	1	CO Physical unit current value / setpoint	Unsigned32	RW	No
0x6407	0	CO Decimal digits current value / setpoint	Unsigned8	RO	No
	1	CO Decimal digits current value / setpoint	Unsigned8	RW	No
0x6410	0	CO Effective controller output Y	Unsigned8	RO	No
	1	CO Effective controller output Y	Unsigned16	RO	Possible
0x6415	0	CO Physical unit controller output	Unsigned8	RO	No
	1	CO Physical unit controller output	Unsigned32	RO	No
0x6420	0	CO Setpoint switch W/W2	Unsigned8	RO	No
	1	CO Setpoint switch W/W2	Boolean	RW	No
0x6421	0	CO Automatic / manual mode A/M	Unsigned8	RO	No
	1	CO Automatic / manual mode A/M	Boolean	RW	No
0x6422	0	CO Controller on / off	Unsigned8	RO	No
	1	CO Controller on / off	Boolean	RW	No
0x6423	0	CO Controller mode	Unsigned8	RO	No
	1	CO Controller mode	Unsigned8	RW	Possible
0x6425	0	CO Control byte	Unsigned8	RO	No
	1	CO Control byte	Unsigned8	RW	Possible
0x6427	0	CO Status word	Unsigned8	RO	No
	1	CO Status word	Unsigned16	RO	Possible
0x7400	0	CO Effective current value Xeff (INT)	Unsigned8	RO	No
	1	CO Effective current value Xeff (INT)	Unsigned16	RW	Possible
0x7401	0	CO Effective setpoint Weff (INT)	Unsigned8	RO	No
	1	CO Effective setpoint Weff (INT)	Unsigned16	RO	Possible
0x7402	0	CO Setpoint W (INT)	Unsigned8	RO	No
	1	CO Setpoint W (INT)	Unsigned16	RW	Possible
0x7403	0	CO 2 nd Setpoint W2 (INT)	Unsigned8	RO	No

Index	Sub Index	Description	Data Type	Access	PDO mapping
	1	CO 2 nd Setpoint W2 (INT)	Unsigned16	RW	Possible
0x7404	0	CO Lower setpoint limit W0 (INT)	Unsigned8	RO	No
	1	CO Lower setpoint limit W0 (INT)	Unsigned16	RO	No
0x7405	0	CO Upper setpoint limit W100 (INT)	Unsigned8	RO	No
	1	CO Upper setpoint limit W100 (INT)	Unsigned16	RO	No

Object 0x6410: CO Effective controller output Y

hexadecimal value	decimal value	percent value
0xFC18	-1000	-100.0%
:::	:::	:::
0xFE0C	-500	-50.0%
:::	:::	:::
0x0000	0	0.0%
:::	:::	:::
0x1F4	500	50.0%
:::	:::	:::
0x3E8	1000	100.0%

0x6422 CO Control On/Off

control byte	Mode
TRUE	DDE parameter 12 control mode = 0 (controller active)
FALSE	DDE parameter 12 control mode = 12 (setpoint 0%)

0x6423 CO Controller mode

control byte	Mode
0x80	manufacturer specific controller type
:::	:::
0xFF	manufacturer specific controller type

Bronkhorst High-Tech B.V. instruments only support range 0x80h – 0x96. It is used as follows:

0x80: DDE parameter 12 control mode = 0
 0x81: DDE parameter 12 control mode = 1
 0x82: DDE parameter 12 control mode = 2
 Etc.

Essential control modes:

Nr.	Mode	Instrument action
0	Controlling	Control at setpoint value
3	Valve closed	No controller action, valve is closed
4	Controller Idle	No controller action, valve remains its position
8	Valve purge	No controller action, valve is fully open



More available control modes can be found in
 "Operation instructions digital instruments" (document nr. 9.17.023).
http://www.bronkhorst.com/en/downloads/instruction_manuals/

0x6425 CO Control byte

MSB					LSB
Reserved		Setpoint switch	Manual Mode	Self-optimisation	Controller on / off
7	4	3			0

Value	Meaning
0	disable function
1	enable function

Self-optimisation is not supported (is always 0)

0x6427 CO Status word

MSB										LSB	
reserved		Net overload	Over-load	Data not valid	reserved		Optimization error	Setpoint switch	Manual Mode	Self-optimization	Controller on / off
15	11	10	9	8	7	5	4	3	2	1	0

Value	Meaning
0	not valid (not occurred)
1	valid (occurred)

The following objects are mapped to the following DDE parameters:

Index	Sub Index	Description	DDE parameter
0x6400	0	CO Effective current value Xeff	-
	1	CO Effective current value Xeff	fMeasure
0x6401	0	CO Effective setpoint Weff	-
	1	CO Effective setpoint Weff	fSetpoint
0x6402	0	CO Setpoint W	-
	1	CO Setpoint W	fSetpoint
0x6403	0	CO 2 nd Setpoint W2	-
	1	CO 2 nd Setpoint W2	-
0x6404	0	CO Lower setpoint limit W0	-
	1	CO Lower setpoint limit W0	Capacity 0% (read only)
0x6405	0	CO Upper setpoint limit W100	-
	1	CO Upper setpoint limit W100	Capacity (read only)
0x6406	0	CO Physical unit current value / setpoint	-
	1	CO Physical unit current value / setpoint	-
0x6407	0	CO Decimal digits current value / setpoint	-
	1	CO Decimal digits current value / setpoint	-
0x6410	0	CO Effective controller output Y	-
	1	CO Effective controller output Y	Valve output (scaled to % as described above)
0x6415	0	CO Physical unit controller output	-
	1	CO Physical unit controller output	-
0x6420	0	CO Setpoint switch W/W2	-
	1	CO Setpoint switch W/W2	-
0x6421	0	CO Automatic / manual mode A/M	-
	1	CO Automatic / manual mode A/M	-
0x6422	0	CO Controller on / off	-
	1	CO Controller on / off	- (is described above)
0x6423	0	CO Controller mode	-
	1	CO Controller mode	Control mode
0x6425	0	CO Control byte	-
	1	CO Control byte	- (is described above)
0x6425	0	CO Status word	-
	1	CO Status word	- (is described above)
0x7400	0	CO Effective current value Xeff (INT)	-
	1	CO Effective current value Xeff (INT)	fMeasure ³

³ Integer16 value scaled with the value of object 0x6407:01

Index	Sub Index	Description	DDE parameter
0x7401	0	CO Effective setpoint Weff (INT)	-
	1	CO Effective setpoint Weff (INT)	fSetpoint ⁵
0x7402	0	CO Setpoint W (INT)	-
	1	CO Setpoint W (INT)	fSetpoint ⁵
0x7403	0	CO 2 nd Setpoint W2 (INT)	-
	1	CO 2 nd Setpoint W2 (INT)	-
0x7404	0	CO Lower setpoint limit W0 (INT)	-
	1	CO Lower setpoint limit W0 (INT)	Capacity 0% (read only) ⁵
0x7405	0	CO Upper setpoint limit W100 (INT)	-
	1	CO Upper setpoint limit W100 (INT)	Capacity (read only) ⁵



The value of object 0x6407:01 CO Decimal digits current value / set point is determined and optimized automatically during instrument power-up.

⁵ Examples:

fMeasure = 1.15 ln/min

object 0x6407:01 CO Decimal digits current value / set point = 3

object 0x7401:01 CO Effective current value Xeff = 1.15 x (10 x 10 x 10) = 1150

object 0x6407:01 CO Decimal digits current value / set point = 4

object 0x7402:01 CO Setpoint W (INT) = 22500

fSetpoint = 22500 / (10 x 10 x 10 x 10) = 2.25 ln/min

⁵ Integer16 value scaled with the value of object 0x6407:01

APPENDIX B: SI UNIT AND PREFIX SPECIFICATION

SI Unit Specification				
Name	Symbol	Notation index (hex)	Index	Description
Kilogram	kg	0x02	0x402	Mass
Second	s	0x03	0x403	Time
Kelvin	K	0x05	0x405	Temperature
Pascal	Pa	0x22	0x422	Pressure
Degree Celcius	°C	0x2D	0x42D	Temperature
Litre	l	0x44	0x444	Volume
Minute	min	0x47	0x447	Time
Hour	h	0x48	0x448	Time
Bar	bar	0x4E	0x44E	Pressure
Cubic metre	m ³	0x59	0x459	Volume

Prefix Specification			
Prefix	Symbol	Factor	Notation Index
<i>reserved</i>	-	-	<i>0x13 – 0x7F</i>
exa	E	10 ¹⁸	0x12
		10 ¹⁷	0x11
		10 ¹⁶	0x10
peta	P	10 ¹⁵	0x0F
		10 ¹⁴	0x0E
		10 ¹³	0x0D
tera	T	10 ¹²	0x0C
		10 ¹¹	0x0B
		10 ¹⁰	0x0A
giga	G	10 ⁹	0x09
		10 ⁸	0x08
		10 ⁷	0x07
mega	M	10 ⁶	0x06
		10 ⁵	0x05
		10 ⁴	0x04
kilo	k	10 ³	0x03
hecto	h	10 ²	0x02
deca	da	10 ¹	0x01
		10 ⁰	0x00
deci	d	10 ⁻¹	0xFF
centi	c	10 ⁻²	0xFE
milli	m	10 ⁻³	0xFD
		10 ⁻⁴	0xFC
		10 ⁻⁵	0xFB
micro	μ	10 ⁻⁶	0xFA
		10 ⁻⁷	0xF9
		10 ⁻⁸	0xF8
nano	n	10 ⁻⁹	0xF7
		10 ⁻¹⁰	0xF6
		10 ⁻¹¹	0xF5
pico	p	10 ⁻¹²	0xF4
		10 ⁻¹³	0xF3
		10 ⁻¹⁴	0xF2
femto	f	10 ⁻¹⁵	0xF1
		10 ⁻¹⁶	0xF0
		10 ⁻¹⁷	0xEF
atto	a	10 ⁻¹⁸	0xEE
<i>reserved</i>	-	-	<i>0xED – 0x80</i>

APPENDIX C: NON-SI UNIT SPECIFICATION

Name	Symbol	Notation index (hex)	Index	Description
gram-force per square centimetre	gf/cm ²	0xA0	0x4A0	pressure
pound-force per square inch	psi	0xA1	0x4A1	pressure
torr pressure	torr	0xA2	0x4A2	pressure
standard atmosphere pressure	atm	0xA3	0x4A3	pressure
meter of water pressure	mH ₂ O	0xA4	0x4A4	pressure
inch of water pressure	``H ₂ O	0xA5	0x4A5	pressure
feet of water pressure	ftH ₂ O	0xA6	0x4A6	pressure
meter of mercury pressure	mHg	0xA7	0x4A7	pressure
inch of mercury pressure	``Hg	0xA8	0x4A8	pressure
cubic centimetre	cc	0xB0	0x4B0	volume
cubic millimetre	mm ³	0xB1	0x4B1	volume
cubic centimetre	cm ³	0xB2	0x4B2	volume
cubic foot per hour	cfh	0xB3	0x4B3	volume
cubic foot per minute	cfm	0xB4	0x4B4	volume
cubic foot per second	cfs	0xB5	0x4B5	volume
litre (normal)	ln	0xC0	0x4C0	volume (normal flow)
cubic centimetre (normal)	ccn	0xC1	0x4C1	volume (normal flow)
cubic millimetre (normal)	mm ³ n	0xC2	0x4C2	volume (normal flow)
cubic centimetre (normal)	cm ³ n	0xC3	0x4C3	volume (normal flow)
cubic metre (normal)	m ³ n	0xC4	0x4C4	volume (normal flow)
standard cubic foot per hour	scfh	0xC5	0x4C5	volume (normal flow)
standard cubic foot per minute	scfm	0xC6	0x4C6	volume (normal flow)
standard cubic foot per second	scfs	0xC7	0x4C7	volume (normal flow)
standard cubic centimetre per minute	sccm	0xC8	0x4C8	volume (normal flow)
standard litre per minute	slm	0xC9	0x4C9	volume (normal flow)
litre (standard)	ls	0xD0	0x4D0	volume (standard flow)
cubic centimetre (standard)	ccs	0xD1	0x4D1	volume (standard flow)
cubic millimetre (standard)	mm ³ s	0xD2	0x4D2	volume (standard flow)
cubic centimetre (standard)	cm ³ s	0xD3	0x4D3	volume (standard flow)
cubic metre (standard)	m ³ s	0xD4	0x4D4	volume (standard flow)